

40-40 Appendix C – CJD Containers

Figure #1 - CJD Waste Receptacle – (Red “Chemotherapy” Waste Bin) SKU #201905.



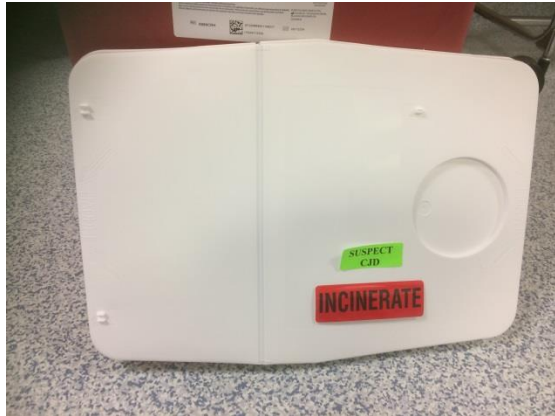


Figure #2 - Lab specimens – Spill-proof, puncture proof sealed container with label. Obtain from Microbiology Lab.

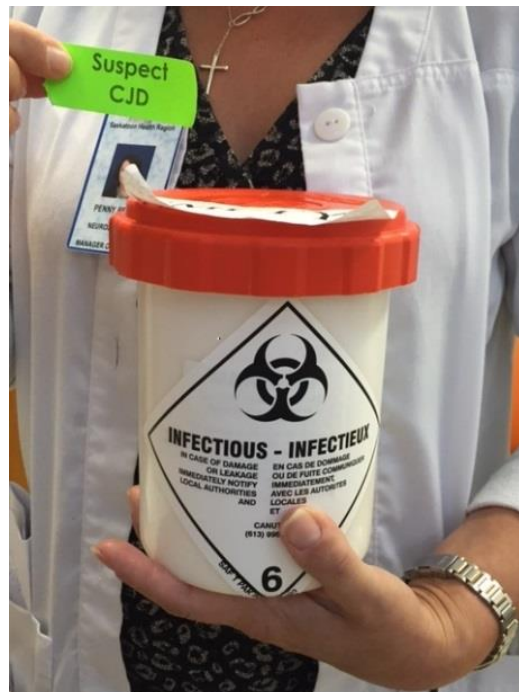

40-40 Appendix C – CJD Containers

Figure #3 – Instrument/Equipment Quarantine for **Suspect** and **Confirmed** CJD diagnosis. RUH “Operating Room” cases.

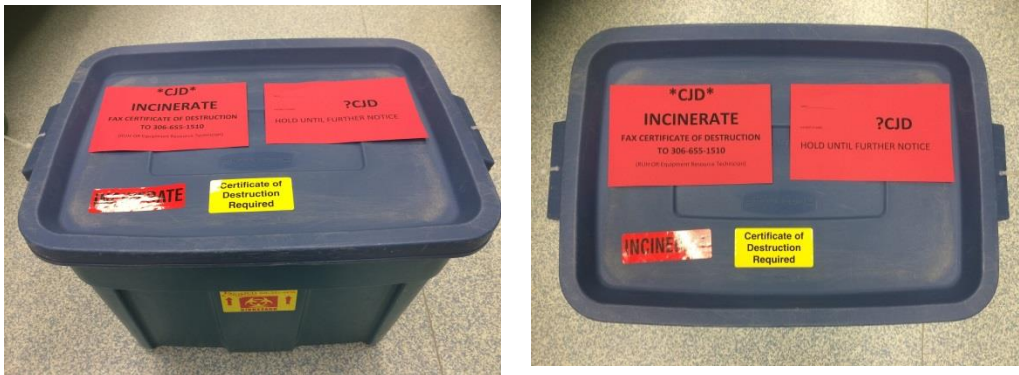

Note: Simply remove the “? CJD – Hold until Further Notice” label if the specimen is positive.